

Data File: C:\LabSolutions\Data\Chemistry\Evans\GF10K-181004-001.lcd


Elmt	Val.	Min	Max	Elmt	Val.	Min	Max	Elmt	Val.	Min	Max	Elmt	Val.	Min	Max	Use Adduct
H	1	50	75	Si	4	0	0	Fe	2	0	0	Ag	1	0	0	H
2H	1	0	0	P	3	0	0	Co	2	0	0	I	3	0	0	Na
C	4	50	65	S	2	0	0	Ni	2	0	0	Re	2	0	0	K
N	3	0	5	Cl	1	0	0	Cu	2	0	0	Ir	3	0	0	NH4
O	2	15	20	V	2	0	0	Br	1	0	0	Pt	2	0	0	
F	1	0	0	Cr	2	0	0	Ru	2	0	0					

Error Margin (ppm): 25
HC Ratio: unlimited
Max Isotopes: all
MSn Iso RI (%): 75.00


DBE Range: -2.0 - 1000.0
Apply N Rule: no
Isotope RI (%): 1.00
MSn Logic Mode: AND

Electron Ions: both
Use MSn Info: yes
Isotope Res: 7000
Max Results: 500


Event#: 1 MS(E+) Ret. Time : 0.079 -> 0.095 - 0.238 -> 0.541 Scan#: 11 -> 13 - 31 -> 69

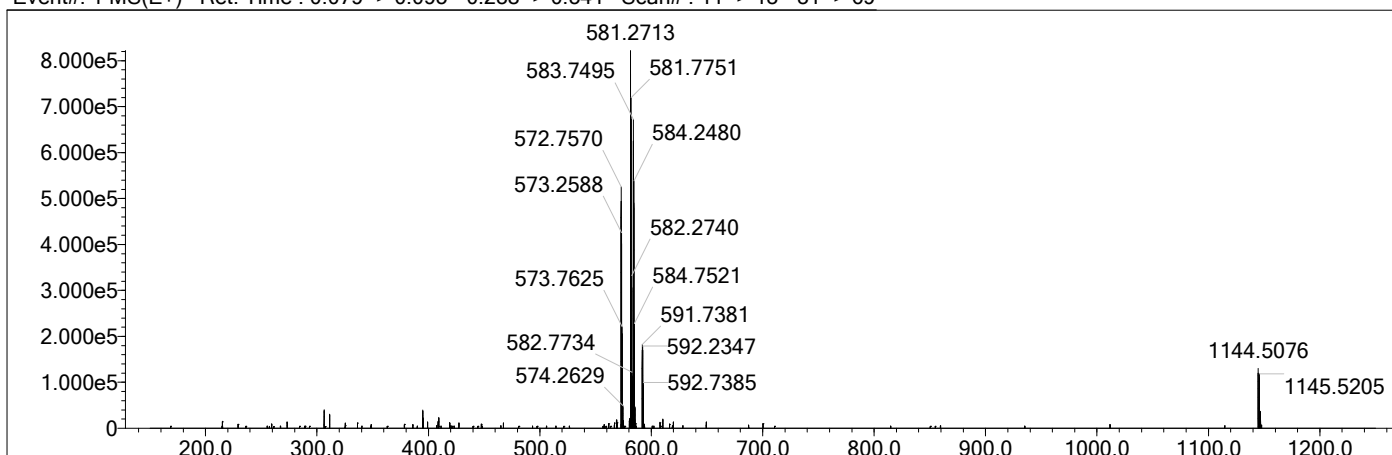

Measured region for 1144.5076 m/z

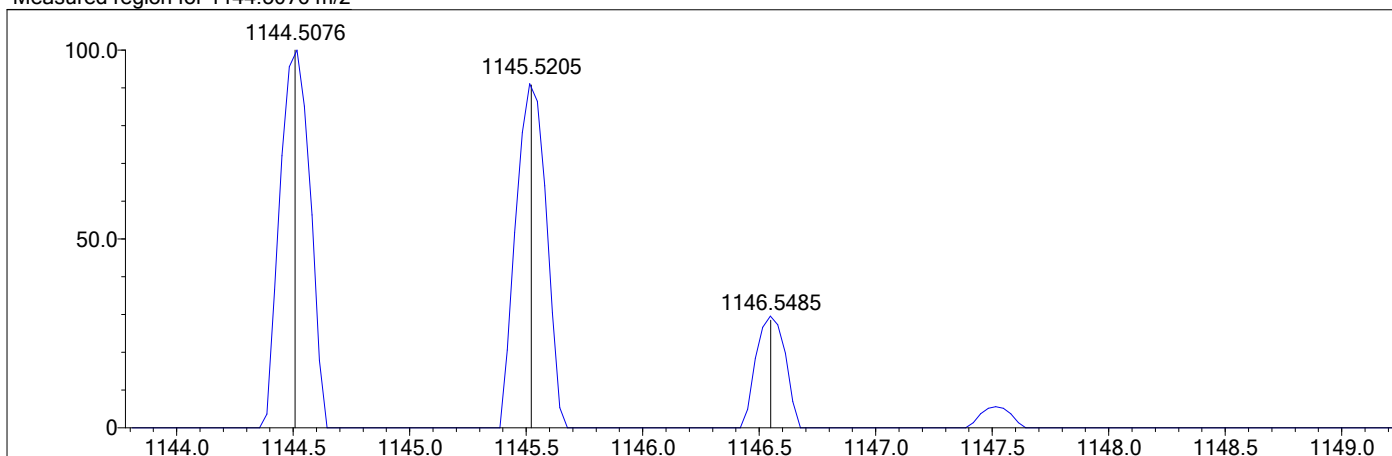

C62 H74 N5 O16 M+ : Predicted region for 1144.5125 m/z

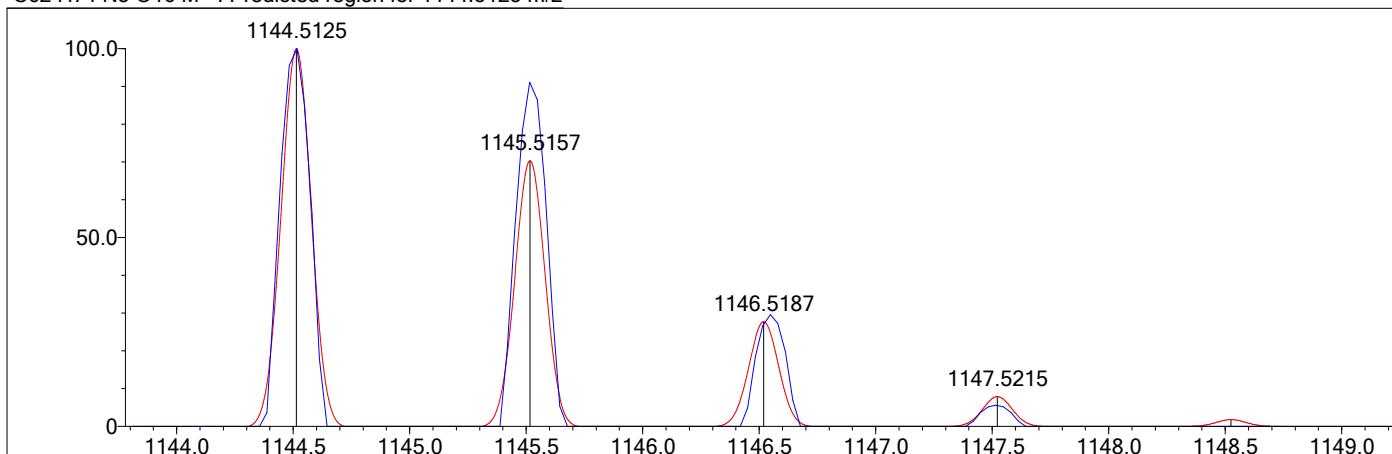

Rank	Score	Formula (M)	Ion	Meas. m/z	Pred. m/z	Df. (mDa)	Df. (ppm)	Iso	DBE
2	39.65	C62 H74 N5 O16	M+	1144.5076	1144.5125	-4.9	-4.28	43.19	28.5