


60 min

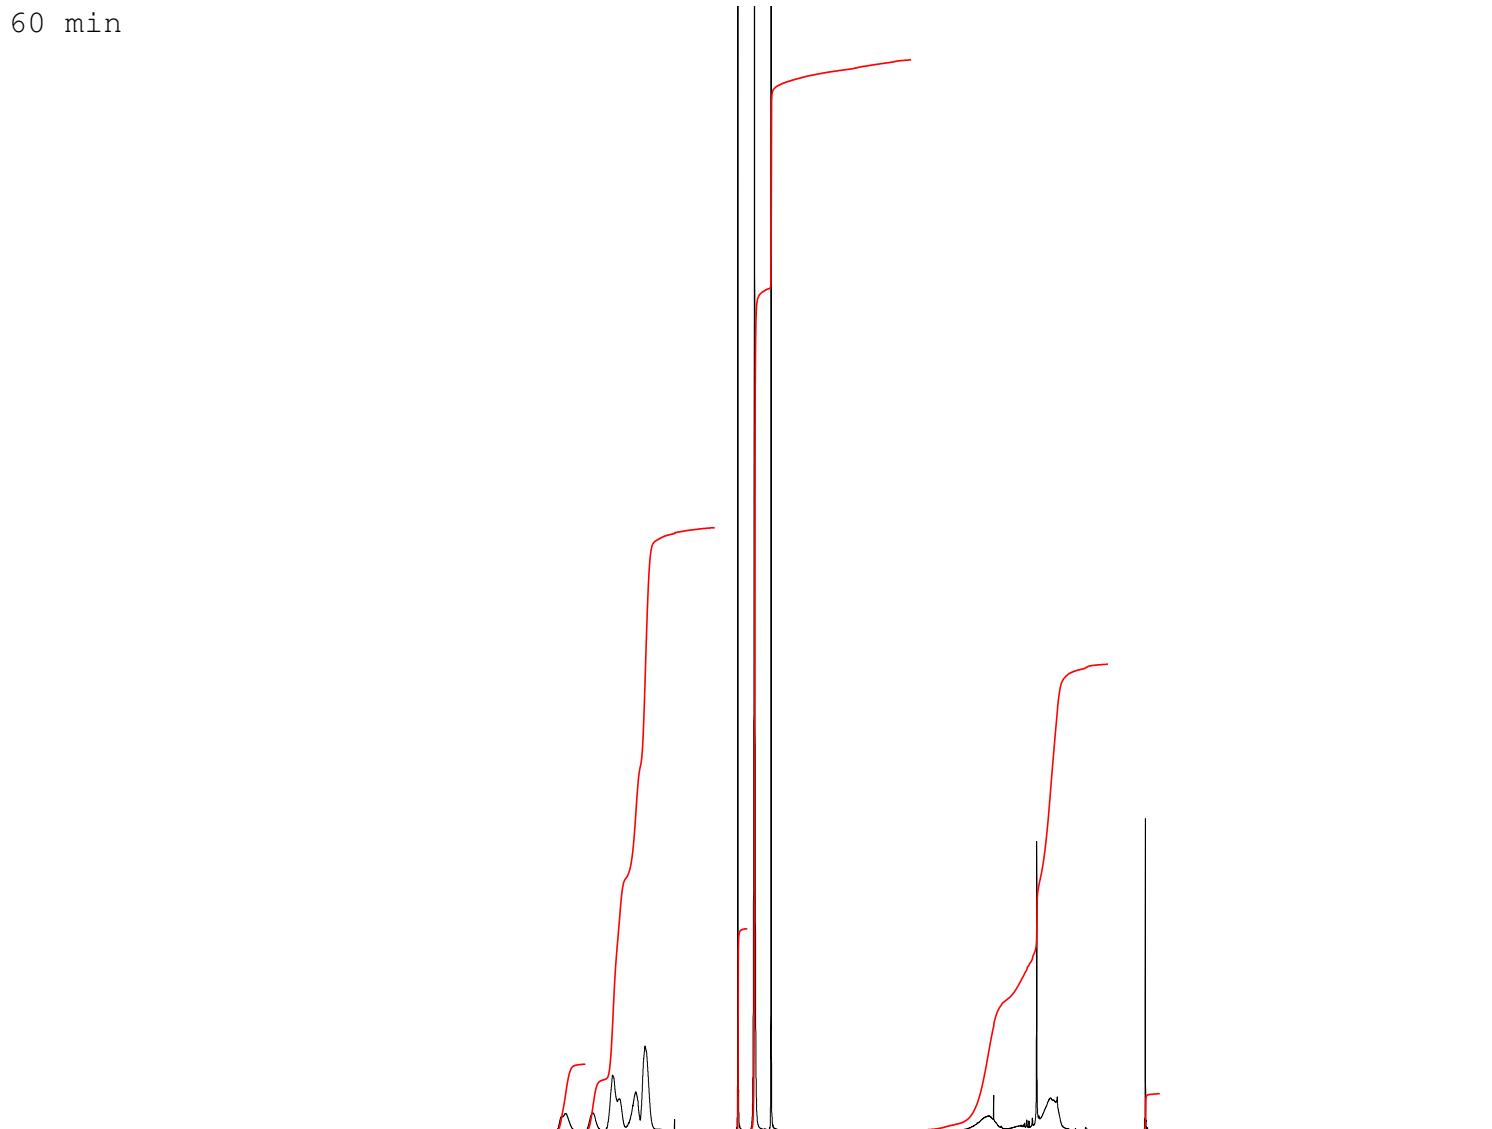

Current Data Parameters  
NAME 2019-02-06-CNW-P1-charging-quartz-r1  
EXPNO 5  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190206  
Time 13.55 h  
INSTRUM AVIII400NB  
PROBHD Z108618\_0022 (   
PULPROG noeipyppr1d  
TD 65536  
SOLVENT CH2Cl2  
NS 8  
DS 4  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894465 sec  
RG 31.99  
DW 62.400 usec  
DE 14.23 usec  
TE 298.0 K  
D1 10.0000000 sec  
D8 0.0100000 sec  
D12 0.00002000 sec  
D16 0.00020000 sec  
TD0 1  
ZGOPTNS -DFLAG\_BLK  
SF01 400.1321240 MHz  
NUC1 1H  
P0 9.87 usec  
P1 9.87 usec  
PLW1 31.29999924 W  
PLW9 0.00000122 W  
GPNAME[1] SMSQ10.100  
GPZ1 50.00 %  
GPNAME[2] SMSQ10.100  
GPZ2 -10.00 %  
P16 1000.00 usec

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

