


# York - Chemistry - Mass Spectrometry Service Report

SB131\_ne0007sb

## Analysis Information

Analysis Filename	ne0007sb_P1-F-2_01_46690.d	Acquisition Date	05/02/2024 08:46:53
Method	ESI_low mass_2c1s.m	Instrument	compact
Submission Name	ne0007sb	ESI	Positive

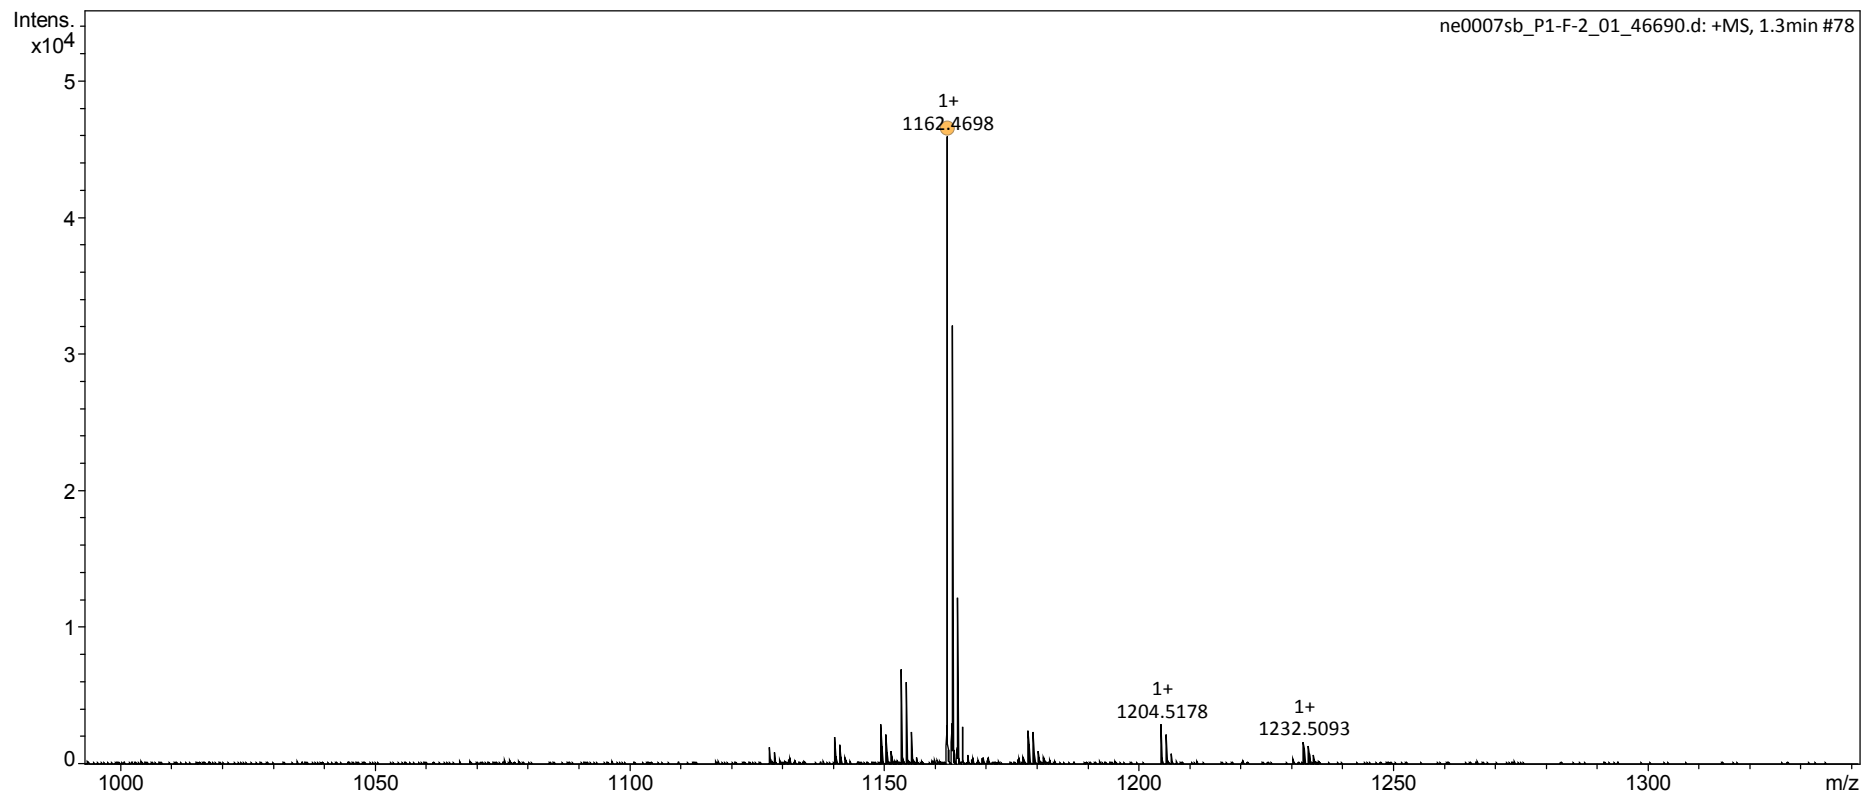

Meas. m/z	#	Ion Formula	m/z	err [ppm]	err [mDa]	mSigma	Mean err [ppm]
1162.4698	1	C <sub>64</sub> H <sub>63</sub> F <sub>6</sub> N <sub>7</sub> NaO <sub>6</sub>	1162.4636	-5.3	-6.1	126.9	-3.1