


York - Chemistry - Mass Spectrometry Service Report

SB141_ne0008sb

Analysis Information

Analysis Filename ne0008sb_P1-F-3_01_46691.d Acquisition Date 05/02/2024 08:54:34
Method ESI_low mass_2c1s.m Instrument compact
Submission Name ne0008sb ESI Positive

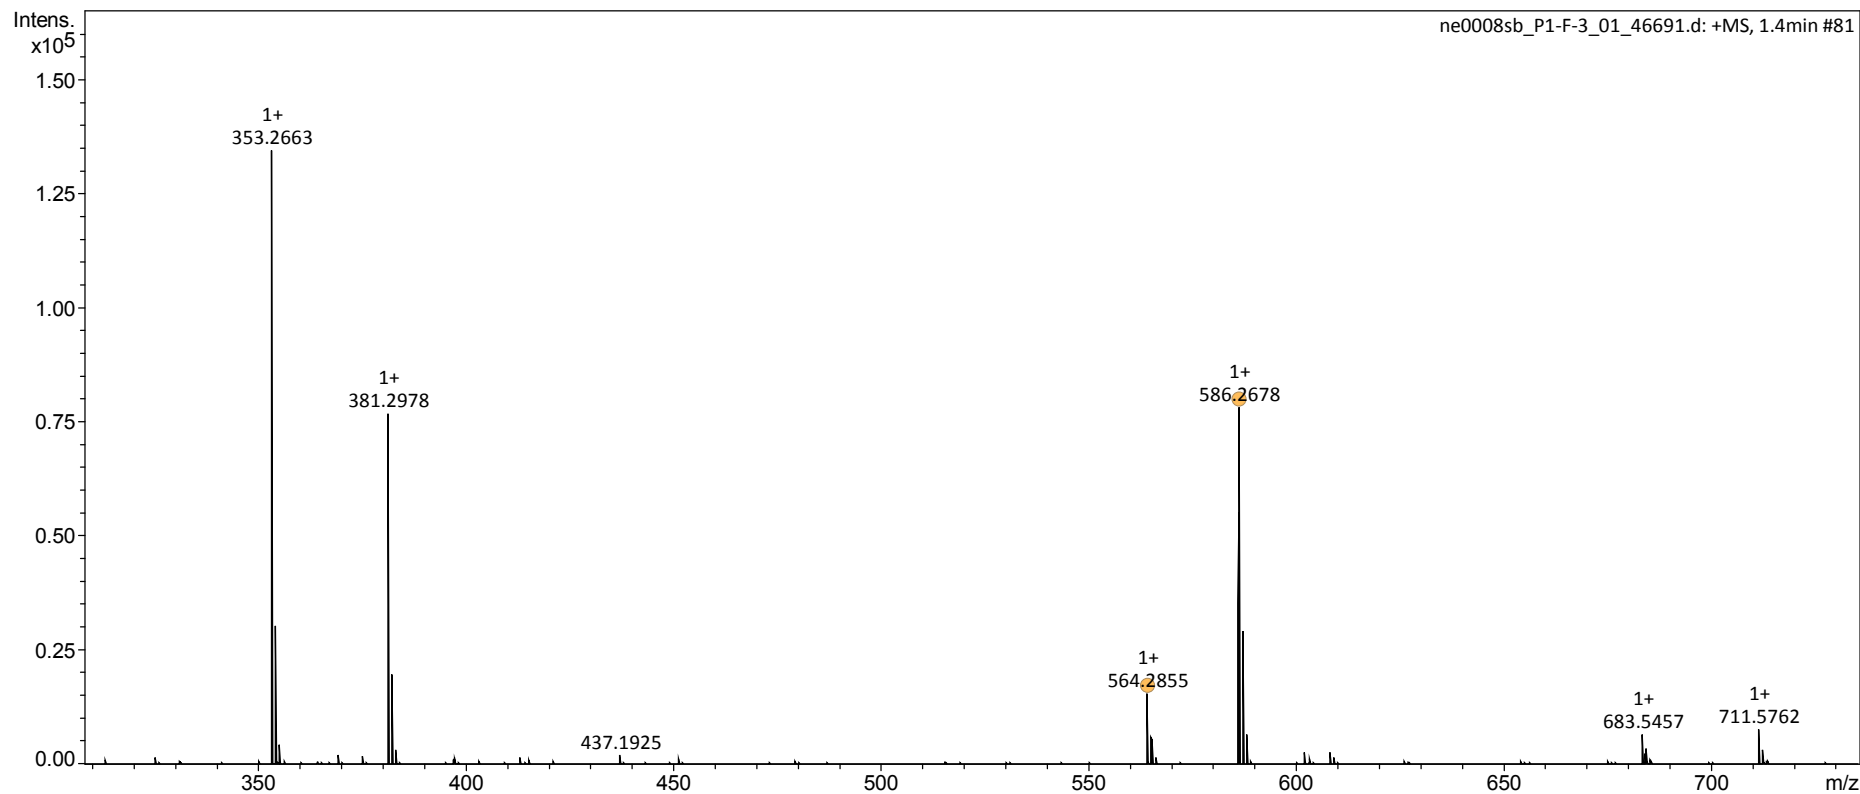

Meas. m/z	#	Ion Formula	m/z	err [ppm]	err [mDa]	mSigma	Mean err [ppm]
564.2855	1	C35H38N3O4	564.2857	0.3	0.1	4.9	0.5
586.2678	1	C35H37N3NaO4	586.2676	-0.3	-0.2	10.3	-0.8